


Biodex Medical Center

55 red st
Shirley, NY 11967

Constancy Test - Activity Report

Printed on: 05/08/2017 1:10:39 PM

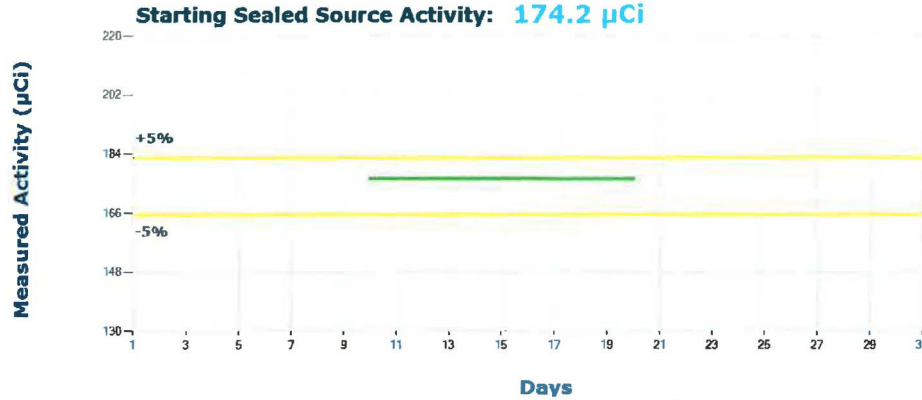

Sealed Source :
Cs-137

Source ID:
BM06S-37-6-2

March 2017

Date	Detector S/N	Measured Activity	Calculated Standard	Acceptable Variance +/- 5 %	Staff
03/31/2017			Test Not Performed		
03/30/2017			Test Not Performed		
03/29/2017			Test Not Performed		
03/28/2017			Test Not Performed		
03/27/2017			Test Not Performed		
03/26/2017			Test Not Performed		
03/25/2017			Test Not Performed		
03/24/2017			Test Not Performed		
03/23/2017			Test Not Performed		
03/22/2017			Test Not Performed		
03/21/2017			Test Not Performed		
03/20/2017	96276013	176.4 μ Ci	174.2 μ Ci	1.3 %	C S
03/20/2017	96276013	176.2 μ Ci	174.2 μ Ci	1.1 %	C S
03/20/2017	96276013	176.2 μ Ci	174.2 μ Ci	1.1 %	C S
03/19/2017			Test Not Performed		
03/18/2017			Test Not Performed		
03/17/2017			Test Not Performed		
03/16/2017			Test Not Performed		
03/15/2017			Test Not Performed		
03/14/2017			Test Not Performed		
03/13/2017			Test Not Performed		
03/12/2017			Test Not Performed		
03/11/2017			Test Not Performed		
03/10/2017	96276013	176.5 μ Ci	174.3 μ Ci	1.3 %	C S
03/10/2017	96276013	176.6 μ Ci	174.3 μ Ci	1.3 %	C S
03/09/2017			Test Not Performed		
03/08/2017			Test Not Performed		
03/07/2017			Test Not Performed		
03/06/2017			Test Not Performed		
03/05/2017			Test Not Performed		
03/04/2017			Test Not Performed		
03/03/2017			Test Not Performed		
03/02/2017			Test Not Performed		
03/01/2017			Test Not Performed		